

DISTRIBUITO IN ITALIA DA:**Meridian Healthcare srl**

Via G. Guglielmino, 68 - 95030 Tremestieri Etneo - CT

Tel. 095 725 68 69 - Fax: 095 725 44 54

e-mail: info@meridianhealthcare.it

 Meridian Healthcare[®]**Instructions for use****Dopamine ELISA** **Fast Track**

Please use only the valid version of the Instructions for use provided with the kit

REF**BA E-6300****IVD****CE**

1. Introduction

1.1 Intended use and principle of the test

Enzyme Immunoassay for the quantitative determination of dopamine in plasma and urine.

Dopamine is extracted by using a cis-diol-specific affinity gel, acylated and then converted enzymatically. The competitive ELISA kit uses the microtiter plate format. The antigen is bound to the solid phase of the microtiter plate. The derivatized standards, controls and samples and the solid phase bound analytes compete for a fixed number of antibody binding sites. After the system is in equilibrium, free antigen and free antigen-antibody complexes are removed by washing. The antibody bound to the solid phase is detected by an anti-rabbit IgG-peroxidase conjugate using TMB as a substrate. The reaction is monitored at 450 nm.

Quantification of unknown samples is achieved by comparing their absorbance with a standard curve prepared with known standard concentrations.

1.2 Clinical application

In humans the catecholamines adrenaline (epinephrine), noradrenaline (norepinephrine) and dopamine are neurotransmitters of the sympathetic nervous system and are involved in many physiological processes. The sympathetic nervous system sets the body to a heightened state of alert, also called as the body's fight-or-flight response.

In the human body the catecholamines and their metabolites indicate the adaption of the body to acute and chronic stress.

Next to the metanephrine/normetanephrine the catecholamines are important for the diagnosis and the follow-up of tumors of the sympathoadrenal system like the pheochromocytomas. The quantitative determination of catecholamines in urine is preferred for the diagnosis of these tumors, whereas the determination of catecholamines in plasma is medically sensible for the localization of the tumor and for function testing. Values above the cut-off can provide an indication for neuroendocrine tumors.

However, in literature various diseases like hypertension, cardiovascular diseases, schizophrenia and manic depression are described with abnormal low or high levels of catecholamines.

Therapeutic consequences should never be based on laboratory results alone even if all test results are in agreement with the items as under point "Procedural cautions, guidelines and warnings". Any laboratory result is only a part of the total clinical picture of the patient.

Only in cases where the laboratory results are in an acceptable agreement with the overall clinical picture of the patient it can be used for therapeutic consequences.

The test result itself should never be the sole determinant for deriving any therapeutic consequences.

2. Procedural cautions, guidelines, warnings and limitations

2.1 Procedural cautions, guidelines and warnings

- (1) This kit is intended for professional use only. Users should have a thorough understanding of this protocol for the successful use of this kit. Only the test instruction provided with the kit is valid and has to be used to run the assay. Reliable performance will only be attained by strict and careful adherence to the instructions provided.
- (2) This assay was validated for certain types of samples as indicated in *Intended Use* (please refer to Chapter 1). Any off-label use of this kit is in the responsibility of the user and the manufacturer cannot be held liable.
- (3) The principles of Good Laboratory Practice (GLP) have to be followed.
- (4) In order to reduce exposure to potentially harmful substances, wear lab coats, disposable protective gloves and protective glasses where necessary.
- (5) All kit reagents and specimens should be brought to room temperature and mixed gently but thoroughly before use. Avoid repeated freezing and thawing of reagents and specimens.
- (6) For dilution or reconstitution purposes, use deionized, distilled, or ultra-pure water.
- (7) The microplate contains snap-off strips. Unused wells must be stored at 2 °C to 8 °C in the sealed foil pouch with desiccant and used in the frame provided.
- (8) Duplicate determination of sample is highly recommended to be able to identify potential pipetting errors.
- (9) Once the test has been started, all steps should be completed without interruption. Make sure that the required reagents, materials and devices are prepared ready at the appropriate time.
- (10) Incubation times do influence the results. All wells should be handled in the same order and time intervals.
- (11) To avoid cross-contamination of reagents, use new disposable pipette tips for dispensing each reagent, sample, standard and control.
- (12) A standard curve must be established for each run.
- (13) The controls should be included in each run and fall within established confidence limits. The confidence limits are listed in the QC-Report provided with the kit.

- (14) Do not mix kit components with different lot numbers within a test and do not use reagents beyond expiry date as shown on the kit labels.
- (15) Avoid contact with Stop Solution containing 0.25 M H₂SO₄. It may cause skin irritation and burns. In case of contact with eyes or skin, rinse off immediately with water.
- (16) TMB substrate has an irritant effect on skin and mucosa. In case of possible contact, wash eyes with an abundant volume of water and skin with soap and abundant water. Wash contaminated objects before reusing them.
- (17) For information on hazardous substances included in the kit please refer to Safety Data Sheet (SDS). The Safety Data Sheet for this product is made available directly on the website of the manufacturer or upon request.
- (18) The expected reference values reported in this test instruction are only indicative. It is recommended that each laboratory establishes its own reference intervals.
- (19) The results obtained with this test kit should not be taken as the sole reason for any therapeutic consequence (e.g. medication before a scheduled surgery) but have to be correlated to other diagnostic tests and clinical observations.
- (20) Kit reagents must be regarded as hazardous waste and disposed according to national regulations.

2.2 Limitations

Any inappropriate handling of samples or modification of this test might influence the results.

2.2.1 Interfering substances

Plasma

Samples containing precipitates or fibrin strands or which are haemolytic or lipemic might cause inaccurate results.

24-hour urine

Please note the sample preparation! If the percentage of the final concentration of acid is too high, this will lead to incorrect results for the urine samples.

2.2.2 Drug interferences

There are no known substances (drugs) which ingestion interferes with the measurement of dopamine level in the sample.

2.2.3 High-Dose-Hook effect

No hook effect was observed in this test.

3. Storage and stability

Store the unopened reagents at 2 - 8 °C until expiration date. Do not use components beyond the expiry date indicated on the kit labels. Once opened the reagents are stable for 1 month when stored at 2 - 8 °C. Once the resealable pouch has been opened, care should be taken to close it tightly with desiccant again.


4. Materials

4.1 Content of the kit

| | | |
|------------------|---|---|
| BA D-0090 | FOILS | Adhesive Foil - Ready to use |
| Content: | Adhesive Foils in a resealable pouch | |
| Volume: | 1 x 4 foils | |
| BA E-0030 | WASH-CONC 50x | Wash Buffer Concentrate - Concentrated 50x |
| Content: | Buffer with a non-ionic detergent and physiological pH | |
| Volume: | 1 x 20 ml/vial, light purple cap | |
| BA E-0040 | CONJUGATE | Enzyme Conjugate - Ready to use |
| Content: | Goat anti-rabbit immunoglobulins, conjugated with peroxidase | |
| Volume: | 1 x 12 ml/vial, red cap | |
| BA E-0055 | SUBSTRATE | Substrate - Ready to use |
| Content: | Chromogenic substrate containing tetramethylbenzidine, substrate buffer and hydrogen peroxide | |
| Volume: | 1 x 12 ml/vial, black cap | |

BA E-0080 **STOP-SOLN** **Stop Solution** - Ready to use

Content: 0.25 M sulfuric acid
 Volume: 1 x 12 ml/vial, light grey cap

Hazards identification: 

H290 May be corrosive to metals.
 H314 Causes severe skin burns and eye damage.

BA E-6310 **DOP-AS** **Dopamine Antiserum** - Ready to use

Content: Rabbit anti-dopamine antibody, green coloured
 Volume: 1 x 6 ml/vial, dark green cap

BA R-0050 **ADJUST-BUFF** **Adjustment Buffer** - Ready to use


Content: TRIS buffer
 Volume: 1 x 4 ml/vial, green cap

Standards and Controls - Ready to use

| Cat. no. | Component | Colour/ Cap | Concentration ng/ml | Concentration nmol/l | Volume/ Vial |
|------------------|--------------|----------------|---|-------------------------|-----------------|
| | | | DOP | DOP | |
| BA E-6601 | STANDARD A | white | 0 | 0 | 4 ml |
| BA E-6602 | STANDARD B | light yellow | 10 | 65 | 4 ml |
| BA E-6603 | STANDARD C | orange | 40 | 261 | 4 ml |
| BA E-6604 | STANDARD D | dark blue | 150 | 980 | 4 ml |
| BA E-6605 | STANDARD E | light grey | 500 | 3 265 | 4 ml |
| BA E-6606 | STANDARD F | black | 2 000 | 13 060 | 4 ml |
| BA E-6609 | STANDARD A/B | light purple | 4.5 | 29 | 4 ml |
| BA E-6651 | CONTROL 1 | light green | Refer to QC report for expected value and acceptable range! | | 4 ml |
| BA E-6652 | CONTROL 2 | dark red | | | 4 ml |

Conversion: Dopamine (ng/ml) x 6.53 = Dopamine (nmol/l)

Content: Acidic buffer with non-mercury stabilizer, spiked with defined quantity of dopamine

 *for the determination of dopamine in plasma the additional **Standard A/B** is mandatory!

BA R-6611 **ACYL-BUFF** **Acylation Buffer** - Ready to use

Content: Buffer with light alkaline pH for the acylation
 Volume: 1 x 20 ml/vial, white cap

BA R-6612 **ACYL-REAG** **Acylation Reagent** - Ready to use

Content: Acylation reagent in DMF and DMSO
 Volume: 1 x 3 ml/vial, light red cap

Hazards identification:   

H360D May damage the unborn child.
 H226 Flammable liquid and vapour.
 H312 + H332 Harmful in contact with skin or if inhaled.
 H319 Causes serious eye irritation.

BA R-6613 **ASSAY-BUFF** **Assay Buffer** - Ready to use

Content: 1M hydrochloric acid and a non-mercury preservative
 Volume: 1 x 6 ml/vial, light grey cap

BA R-6614 **COENZYME** **Coenzyme** - Ready to use

Content: S-adenosyl-L-methionine
 Volume: 1 x 4 ml/vial, purple cap

BA R-6615 ENZYME **Enzyme** - Lyophilized

Content: Catechol-O-methyltransferase

Volume: 2 vials, pink cap

BA R-6617 EXTRACT-BUFF **Extraction Buffer** - Ready to use

Content: Buffer containing carbonate

Volume: 1 x 6 ml/vial, brown cap

BA R-6618 EXTRACT-PLATE 48 **Extraction Plate** - Ready to use

Content: 2 x 48 well plates coated with boronate affinity gel in a resealable pouch

BA R-6619 HCL **Hydrochloric Acid** - Ready to use

Content: 0.025 M Hydrochloric Acid, yellow coloured

Volume: 1 x 20 ml/vial, dark green cap

BA E-0331 DOP **Dopamine Microtiter Strips**- Ready to use

Content: 1 x 96 well (12x8) antigen precoated microwell plate in a resealable green pouch with desiccant

4.2 Additional materials and equipment required but not provided in the kit

- Calibrated precision pipettes to dispense volumes between 10 – 700 µl; 1 ml
- Microtiter plate washing device (manual, semi-automated or automated)
- ELISA reader capable of reading absorbance at 450 nm and if possible 620 - 650 nm
- Microtiter plate shaker (shaking amplitude 3 mm; approx. 600 rpm)
- Absorbent material (paper towel)
- Water (deionized, distilled, or ultra-pure)
- Vortex mixer

5. Sample collection and storage

Plasma

Whole blood should be collected into centrifuge tubes containing EDTA as anti-coagulant (Monovette™ or Vacuette™ for plasma) and centrifuged according to manufacturer's instructions immediately after collection. Haemolytic and lipemic samples should not be used for the assay.

Storage: up to 6 hours at 2 - 8 °C, for longer period (up to 6 month) at -20 °C.

Repeated freezing and thawing should be avoided.

Urine

Spontaneous urine or 24-hour urine, collected in a bottle containing 10 - 15 ml of 6 M HCl, can be used.

If 24-hour urine is used please record the total volume of the collected urine.

Storage: up to 48 hours at 2 - 8 °C, up to 24 hours at room temperature, for longer periods (up to 6 month) at -20 °C. Repeated freezing and thawing should be avoided.

Avoid exposure to direct sunlight.

6. Test procedure

Allow all reagents to reach room temperature and mix thoroughly by gentle inversion before use. Duplicate determinations are recommended. It is recommended to number the strips of the microwell plate before usage to avoid any mix-up.

The binding of the antiserum and the enzyme conjugate and the activity of the enzyme used are temperature dependent, and the absorbance may vary if a thermostat is not used. The higher the temperature, the higher the absorbance will be. Varying incubation times will have a similar influence on the absorbance. The optimal temperature during the Enzyme Immunoassay is between 20 – 25 °C.

6.1 Preparation of reagents

Wash Buffer

Dilute the 20 ml Wash Buffer Concentrate with water (deionized, distilled, or ultra-pure) to a final volume of 1000 ml.

Storage: 1 month at 2 – 8 °C

Enzyme Solution

Reconstitute the content of the vial labelled 'Enzyme' with 1 ml water (deionized, distilled, or ultra-pure) and mix thoroughly. Add 0.3 ml of Coenzyme followed by 0.7 ml of Adjustment Buffer. The total volume of the Enzyme Solution is 2.0 ml.

⚠ *The Enzyme Solution has to be prepared freshly prior to the assay (not longer than 10 - 15 minutes in advance). Discard after use!*

Dopamine Microtiter Strips

In rare cases residues of the blocking and stabilizing reagent can be seen in the wells as small, white dots or lines. These residues do not influence the quality of the product.

6.2 Sample preparation, extraction and acylation

⚠ **for the determination of dopamine in plasma the additional **Standard A/B** is mandatory!*

| | |
|-----|---|
| 1. | Pipette 10 µl of standards, controls, urine samples and 300 µl of plasma samples into the respective wells of the Extraction Plate . |
| 2. | Add 250 µl of water (deionized, distilled, or ultra-pure) to the wells with standards, controls and urine samples . |
| 3. | Pipette 50 µl of Assay Buffer into all wells. |
| 4. | Pipette 50 µl of Extraction Buffer into all wells. |
| 5. | Cover plate with Adhesive Foil and incubate 30 min at RT (20 – 25 °C) on a shaker (approx. 600 rpm). |
| 6. | Remove the foil. Empty plate and blot dry by tapping the inverted plate on absorbent material. |
| 7. | Pipette 1 ml of Wash Buffer into all wells. Incubate the plate for 5 min at RT (20 – 25 °C) on a shaker (approx. 600 rpm). Empty plate and blot dry by tapping the inverted plate on absorbent material. |
| 8. | Pipette another 1 ml of Wash Buffer into all wells. Incubate the plate for 5 min at RT (20 – 25 °C) on a shaker (approx. 600 rpm). Empty plate and blot dry by tapping the inverted plate on absorbent material. |
| 9. | Pipette 150 µl of Acylation Buffer into all wells. |
| 10. | Pipette 25 µl of Acylation Reagent into all wells. |
| 11. | Incubate 15 min at RT (20 – 25 °C) on a shaker (approx. 600 rpm). |
| 12. | Empty plate and blot dry by tapping the inverted plate on absorbent material. |
| 13. | Pipette 1 ml of Wash Buffer into all wells. Incubate the plate for 10 min at RT (20-25°C) on a shaker (approx. 600 rpm). Empty plate and blot dry by tapping the inverted plate on absorbent material. |
| 14. | Pipette 175 µl of Hydrochloric Acid into all wells. |
| 15. | Cover plate with Adhesive Foil . Incubate 10 min at RT (20 – 25 °C) on a shaker (approx. 600 rpm). Remove the foil and discard. Do not decant the supernatant thereafter! |

⚠ The following volumes of the supernatant are needed for the subsequent ELISA:

| | | | |
|-------------------------------------|--------------|--------------------------|--------------|
| Dopamine (standards + urine) | 25 µl | Dopamine (plasma) | 50 µl |
|-------------------------------------|--------------|--------------------------|--------------|

6.3 Dopamine ELISA

| | |
|-----|---|
| 1. | Pipette 25 µl of the Enzyme Solution (refer to 6.1) into all wells of the Dopamine Microtiter Strips . |
| 2. | Pipette 25 µl of the extracted standards, controls, urine samples and 50 µl of the extracted plasma samples into the appropriate wells. |
| 3. | Add 25 µl of Hydrochloric Acid to the standards, controls and urine samples . |
| 4. | Incubate for 30 min at RT (20 – 25 °C) on a shaker (approx. 600 rpm). |
| 5. | Pipette 50 µl of the Dopamine Antiserum into all wells and cover plate with Adhesive Foil . |
| 6. | Incubate for 2 h at RT (20 – 25 °C) on a shaker (approx. 600 rpm). |
| 7. | Remove the foil. Discard or aspirate the content of the wells. Wash the plate 3 x by adding 300 µl of Wash Buffer , discarding the content and blotting dry each time by tapping the inverted plate on absorbent material. |
| 8. | Pipette 100 µl of the Enzyme Conjugate into all wells. |
| 9. | Incubate for 30 min at RT (20 – 25 °C) on a shaker (approx. 600 rpm). |
| 10. | Discard or aspirate the content of the wells. Wash the plate 3 x by adding 300 µl of Wash Buffer , discarding the content and blotting dry each time by tapping the inverted plate on absorbent material. |
| 11. | Pipette 100 µl of the Substrate into all wells and incubate for 25 ± 5 min at RT (20 – 25 °C) on a shaker (approx. 600 rpm). ⚠ Avoid exposure to direct sun light! |
| 12. | Add 100 µl of the Stop Solution to each well and shake the microtiter plate to ensure a homogeneous distribution of the solution. |
| 13. | Read the absorbance of the solution in the wells within 10 minutes, using a microplate reader set to 450 nm (if available a reference wavelength between 620 nm and 650 nm is recommended). |

7. Calculation of results

| Measuring range | Dopamine | |
|-----------------|-------------------|-------------------|
| | Urine | 4.8 – 2 000 ng/ml |
| Plasma | 75 – 33 333 pg/ml | |

The standard curve is obtained by plotting the absorbance readings (calculate the mean absorbance) of the standards (linear, y-axis) against the corresponding standard concentrations (logarithmic, x-axis).

Use a non-linear regression for curve fitting (e.g. spline, 4- parameter, akima).

⚠ *This assay is a competitive assay. This means: the OD-values are decreasing with increasing concentrations of the analyte. OD-values found below the standard curve correspond to high concentrations of the analyte in the sample and have to be reported as being positive.*

Urine samples and controls

The concentrations of the **urine samples** and the **Controls 1 and 2** can be read directly from the standard curve.

Calculate the 24 h excretion for each urine sample: **µg/24h = µg/l x l/24h**

Plasma samples

The read concentrations of the **plasma samples** have to be **divided by 60**.

Conversion

Dopamine (ng/ml) x 6.53 = Dopamine (nmol/l)

Expected reference values


It is strongly recommended that each laboratory should determine its own normal and abnormal values.


| | Dopamine |
|---------------|----------------------------------|
| 24-hour urine | < 600 µg/day (3 900 nmol/day) |
| Plasma | < 100 pg/ml |

7.1 Quality control

It is recommended to use control samples according to national regulations. Use controls at both normal and pathological levels. The kit or other commercial controls should fall within established confidence limits. The confidence limits of the kit controls are printed on the QC-Report.

7.2 Typical standard curve

 Example, do not use for calculation!

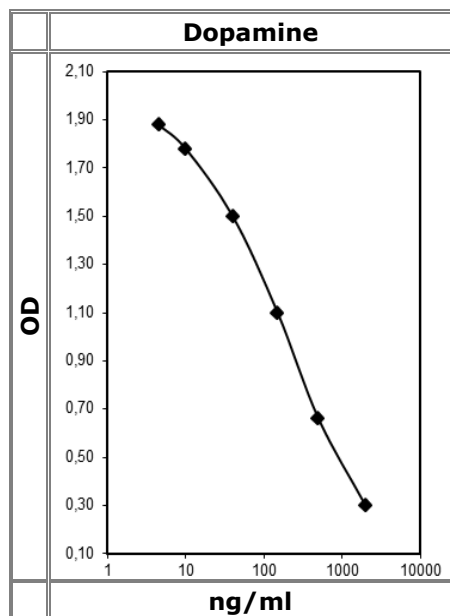

8. Assay characteristics

| Analytical Sensitivity | LOD | Dopamine | |
|------------------------|----------------|---------------|-----|
| | | Urine (ng/ml) | 2.5 |
| | Plasma (pg/ml) | 49 | |
| | LOQ | Urine (ng/ml) | 4.8 |
| Plasma (pg/ml) | | 75 | |

| Analytical Specificity (Cross Reactivity) | Substance | Cross Reactivity (%) | |
|---|--|----------------------|-----|
| | | Dopamine | 100 |
| | Derivatized Adrenaline | 0.02 | |
| | Derivatized Noradrenaline | 6.4 | |
| | Derivatized Dopamine | 100 | |
| | Metanephrine | < 0.01 | |
| | Normetanephrine | 0.01 | |
| | 3-Methoxytyramine | 0.49 | |
| | 3-Methoxy-4-hydroxyphenylglycol | < 0.01 | |
| | Tyramine | 0.18 | |
| | Phenylalanine, Caffeinic acid, L-Dopa, Homovanillic acid, Tyrosine, 3-Methoxy-4-hydroxymandelic acid | < 0.01 | |

| Precision | | | | | | | |
|----------------------------|--------|---------------|--------|-----------------------------|--------|---------------|--------|
| Intra-Assay Urine (n = 60) | | | | Intra-Assay Plasma (n = 60) | | | |
| | Sample | Range (ng/ml) | CV (%) | | Sample | Range (pg/ml) | CV (%) |
| Dopamine | 1 | 82 ± 16.1 | 19.7 | Dopamine | 1 | 75 ± 22 | 29.8 |
| | 2 | 253 ± 41.1 | 16.3 | | 2 | 353 ± 86 | 24.4 |
| | 3 | 714 ± 67 | 9.4 | | 3 | 1187 ± 293 | 24.9 |
| Inter-Assay Urine (n = 33) | | | | Inter-Assay Plasma (n = 18) | | | |
| | Sample | Range (ng/ml) | CV (%) | | Sample | Range (pg/ml) | CV (%) |
| Dopamine | 1 | 79.3 ± 18.8 | 23.7 | Dopamine | 1 | 238 ± 67.0 | 28.2 |
| | 2 | 222 ± 27.0 | 12.1 | | 2 | 1072 ± 201 | 18.8 |
| | 3 | 630 ± 69.0 | 11.0 | | 3 | 3449 ± 491 | 14.2 |

| Linearity | | | Serial dilution up to | Range (%) | Mean (%) |
|-----------|----------|-------|-----------------------|-----------|----------|
| | Dopamine | Urine | | 1:512 | 83 - 126 |
| Plasma | | | 1:512 | 85 - 132 | 106 |

| Recovery | | | Mean (%) | Range (%) | Range |
|----------|----------|-------|----------|-----------|---------------------|
| | Dopamine | Urine | | 110 | 101 - 124 |
| Plasma | | | 89 | 84 - 92 | 57.4 – 16 054 pg/ml |












9. References/Literature

- (1) Kim et al. Vitamin C prevents stress-induced damage on the heart caused by the death of cardiomyocytes, through the down-regulation of the excessive production of catecholamine, TNF- α , and ROS production in GULO(-I-) Vit C-Insufficient mice. Free Radical Biology and Medicine, 65:573-583 (2013)
- (2) Bada et al. Peripheral vasodilatation determines cardiac output in exercising humans: insight from atrial pacing. The Journal of Physiology, 590(8):2051-2060 (2012)
- (3) Parks et al. Employment and work schedule are related to telomere length in women. Occupational & Environmental Medicine 68(8):582-589 (2011)

Please use only the valid version of the Instructions for Use provided with the kit

 **For updated literature or any other information please contact your local supplier.**

Symbols:

| | | | | | |
|---|------------------------------|---|------------------|---|-----------------------------------|
|  | Storage temperature |  | Manufacturer |  | Contains sufficient for <n> tests |
|  | Expiry date |  | Batch code |  | For in-vitro diagnostic use only! |
|  | Consult instructions for use |  | Content |  | CE labelled |
|  | Caution |  | Catalogue number | | |